

January 31, 1974

Communications to the Editor should be addressed to Board of Editors, The Physico-Chemical Society of Japan, Faculty of Science, Kyoto University, Kyoto, Japan

Business Correspondences should be addressed to: Secretary, The Physico-Chemical Society of Japan, Faculty of Science, Kyoto University, Kyoto, Japan.

Purchase Order should be addressed to: Maruzen Co., Ltd., Nihonbashi, Chuo-ku, Tokyo, Japan.

Published by


THE PHYSICO-CHEMICAL SOCIETY OF JAPAN

(Nippon Butsuri-Kagaku Kenkyu Kai)

Faculty of Science, Kyoto University, Kyoto, Japan

Printed by KAWAKITA PRINTING CO., LTD., Kyoto, Japan

KS TYPE SUPER-HIGH -PRESSURE APPARATUS

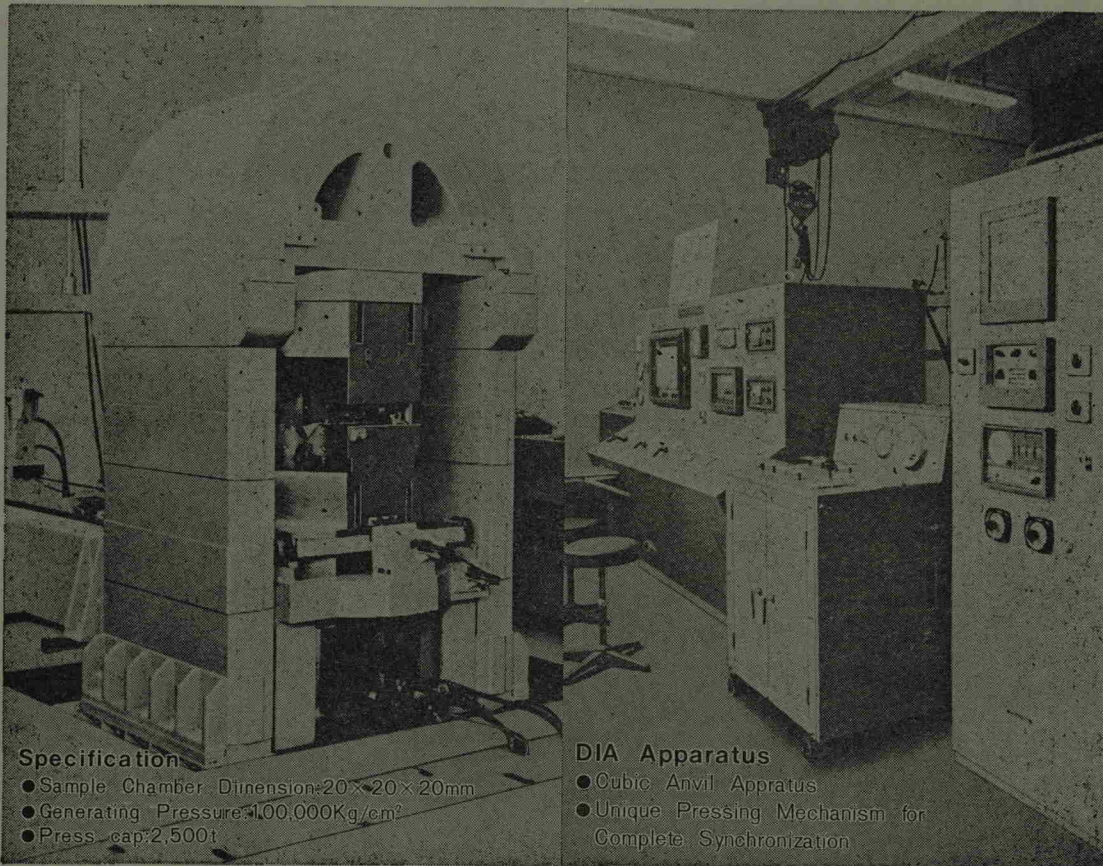

Specification

- Sample Chamber Dimension: 20×20×20mm
- Generating Pressure: 100,000Kg/cm²
- Press. cap: 2,500t

DIA Apparatus

- Cubic Anvil Apparatus
- Unique Pressing Mechanism for Complete Synchronization

**(Fluid Pressure up to 20,000Kg/cm²
Solid Pressure up to 100,000Kg/cm²)**

- Super-High-Pressure Generator
- High-Pressure High-Temperature Apparatus
- High-Pressure Gauge
- Various Super-High-Pressure Systems



KOBE STEEL
MACHINERY DIVISION

Tokyo Office: Tekko Building, 8-2, 1-chome, Marunouchi, Chiyoda-ku, Tokyo, Japan Phone: Tokyo (03) 218-7111
Düsseldorf Office: Immermannstr. 10, 4000 Düsseldorf, West Germany Phone: (0211) 358020, 364550

New York Office: 529 Fifth Avenue, New York, N.Y. 10017, U.S.A. Phone: (212) 867-9710/6

Chicago Office: 111 East Wacker Drive, Chicago, Ill. 60601, U.S.A. Phone: (312) 644-2235/9