

## 2.2. Temperature scale

The thermometer was a 10  $\Omega$ , 1 W, Allen-Bradley carbon resistor; its plastic cover was ground off and the resistor then placed inside its cavity with varnish. It was calibrated against the vapour pressures of helium ( $^4\text{He}$ ) and hydrogen (of known ortho-para composition) close to their normal boiling points. For interpolation the two-constant formula (Clement 1955) was used,

$$\left(\frac{\log R}{T_c}\right)^{\frac{1}{2}} = a + b \log R, \quad (1)$$

where  $R$  is the resistance and the constants  $a$  and  $b$  are determined from the calibration points. Temperatures as determined from equation (1) are for clarity designated by  $T_c$ .

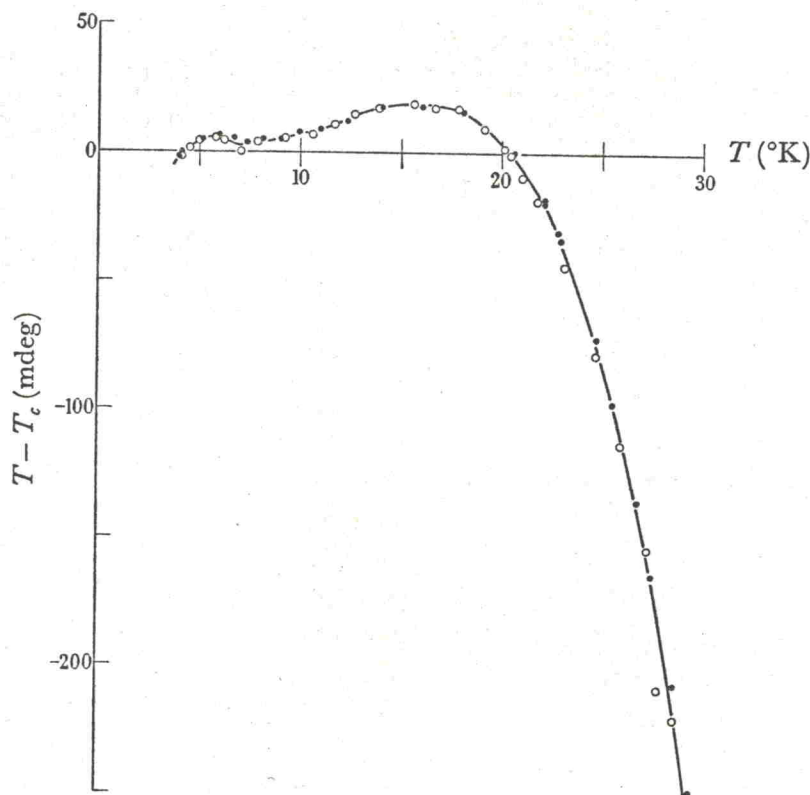


FIGURE 3. Corrections applied to the carbon thermometer temperature  $T_c$  to convert it to the absolute temperature  $T$ .

This calibration was performed each time after the thermometer had been allowed to warm up to room temperature and a slight change of the constants  $a$  and  $b$  was observed after each warm-up.

It is known that interpolation with equation (1) leads to serious deviations from true temperature, especially above 20 °K. A complete calibration of the thermometer against the helium gas thermometer was therefore obtained. The technique employed was as described by Franck & Martin (1961). Temperatures as obtained from the gas thermometer readings are designated  $T$  and are believed to be accurate to within  $\pm 5$  mdeg. The results of two calibrations are given in figure 3 as  $T - T_c$  plotted against  $T$ .

From previous experience with thermometers of the Allen-Bradley type it was known that the effect of successive warm-ups on the deviation curve  $T - T_c$  is almost negligible