

## 2.2. Method of RC balance.

Two methods were adopted to establish the condition

$$R_s C_s = R_r C_r.$$

### a) Reference resistor at a fixed temperature.

This method is a conventional one [1]. By means of the second channel, 30 kHz wide, centered at 455 kHz, the two noise signals were balanced.

### b) Reference resistor at an elevated temperature.

This new method is appropriate to the high pressure use. The temperature  $T_r$  at the atmospheric pressure was equalized to the temperature  $T_s$  under high pressure, until  $N_s$  was consistent with  $N_r$  under the condition  $R_s = R_r$ . When  $R_s = R_r$ , the balance of the real parts of the parallel combination of  $R_s$  and  $C_s$  leads to the condition

$$R_s C_s = R_r C_r.$$

This balance condition was easily attained by means of an AC bridge.

## 2.3. Sensing resistor.

A ceramic-moulded solid carbon resistor made by Allen and Bradley was used as a sensing resistor. The resistor has advantages claimed for the use in the confined environment of high pressure and high temperature. The resistor was shielded completely by a copper tube as shown in Fig. 2. The estimated current noise of the sensing resistor by a grid current is  $0.05 \mu\text{V}$  at most. The comparison between the thermal noise of the sensing resistor and that of the metal wire indicates a good agreement within the limit of error.

## 2.4. Pressure generator.

A girdle type press was employed in this experiment as the high temperature and high pressure generator. Fig. 2 shows the assembly of the pressure cell. The sensing resistor passing through the core of the anvil was brought into contact with the thermocouple at the center of the pressure cell. The temperature difference between the sensing resistor and the thermocouple was estimated within  $\pm 0.8 \text{ K}$  at  $700 \text{ K}$ . To avoid the induction noise arising from the heater, DC current from the battery was applied.

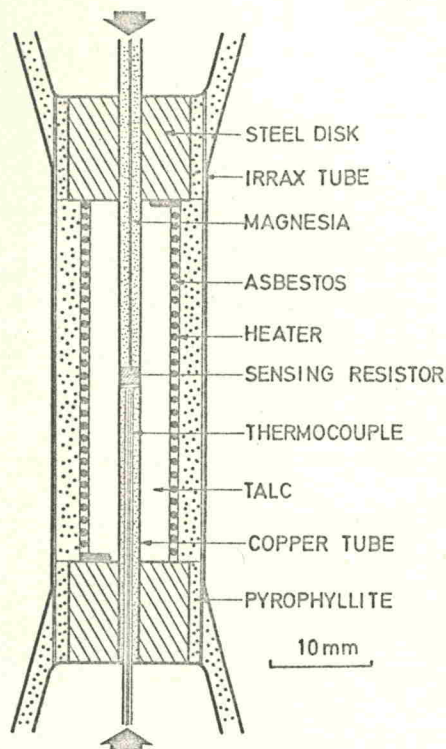


FIG. 2  
Pressure cell assembly.

## 3. Results and discussion

### 3.1. Experimental confirmation of pressure independence of the noise thermometry.

The theoretical statement that the output of the noise thermometer does not depend on the pressure was confirmed experimentally up to 30 kbar at room temperature as listed in Table 1.

### 3.2. Pressure effects on the outputs of Chr/Alu and Cu/Const thermocouples.

The thermometry with the balancing method (b) was applied to the correction of Chr/Alu thermocouple at an elevated temperature. The precise balancing point of  $N_s$  and  $N_r$  was determined from reading the count-integrator over a period of 60 s.  $R_s$  was about  $600 \Omega$  under high pressure. The plotted points in Fig. 3 are the average values of 5 ~ 10 measurements. The result was converted to the standard pressure correction of the thermocouple introduced into a hydrostatic pressure