

## METHODS AND TECHNIQUES OF PHYSICO-CHEMICAL RESEARCH

U.D.C. 541./545

### Tube for the Investigation of Gas-Liquid Heterogeneous Systems at Ultrahigh Pressures

N.A. Grigor'ev, G.P. Shakhovskoi,  
Sh.A. Karapetyan, and B.A. Englin

An unsealed metallic tube fixed in a steel shell with a removable valve and a mobile piston has been designed and tested. The space between the walls of the tube and the shell is filled with silicone oil, which provides a hydraulic support for the tube. Lead tubes and bellows-type and smooth stainless steel tubes have been tested. The telomerisation of ethylene by polychloromethanes has been investigated in the tube at a pressure of 2400 atm and 95°C.


Tubes made of glass (with a mercury seal<sup>1</sup>), lead<sup>2</sup>, Teflon<sup>3</sup>, and mild steel<sup>4</sup> are used for the investigation of liquid-phase processes at high and ultrahigh pressures; the tubes are placed in the reactor of the apparatus filled with a pressure-transmitting liquid. However, these tubes are unsuitable for the investigation of gas-liquid heterogeneous systems, since at fairly high temperatures the initial pressure within the tubes may reach several hundreds of atmospheres. Nor can one use in such investigations the sealed tube with a mobile piston described by Gonikberg and Gavrilova<sup>5</sup>.

We designed and tested an unsealed metallic tube fixed in a steel shell with a removable valve and a mobile ground piston (see Figure). The space between the walls of the tube and the shell is filled with a silicone oil, which provides a hydraulic support for the tube. The telomerisation of ethylene by polychloromethanes was investigated in this tube at a pressure of 2400 atm and a temperature of 95°C<sup>7</sup>. The high-pressure apparatus was described previously<sup>2</sup>.

Successful tests were performed on lead tubes and corrugated (bellows-type) (wall thickness 0.1 mm) and smooth (wall thickness 0.3 mm) stainless steel tubes. Tubes made of polymeric materials (Teflon) proved to be unsuitable because of the permeability of the walls to gas at a high partial pressure.

The Figure shows the steel shell with a lead tube, the upper part of which was rolled out and sealed between the shell and the head. The steel tubes were sealed by means of a sealing ring with a tail piece welded to the neck of the tube. The experimental technique, which was the same for all the tubes, consisted of the following observations. Silicone oil was poured into the steel shell and the tube, closed by a stopper, was inserted. The excess oil was removed, the neck of the tube was washed, and the head was screwed on. The tube was weighed together with the needle valve. Then the liquid telogen was introduced, the needle valve was screwed shut, and the tube was joined to a permanently fixed three-way connector. Then a rotatory spanner and a locking bracket were inserted, the telogen was freed from traces of oxygen by repeated freezing and unfreezing, the tube was disconnected, and the amount of telogen introduced was determined by

reweighing. Next the tube was reconnected to the three-way connector and the spanner and the locking bracket were reintroduced. The tube was filled via the side arm of the three-way connector with ethylene freed from traces of oxygen by repeated freezing and unfreezing, the needle valve was screwed shut, the spanner was removed, and the tube was disconnected. The amount of ethylene added was found by weighing.

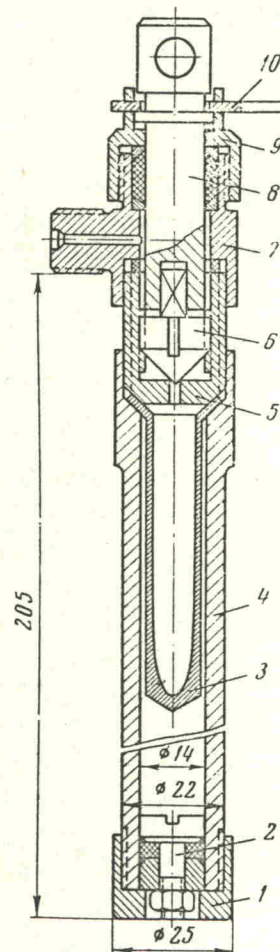

Apparatus for the high-pressure measurements  
1) lock nut; 2) demountable moving piston operating on for principle of a seal with an uncompensated area<sup>6</sup>; 3) tube; 4) shell of tube; 5) head; 6) locking needle valve; 7) three-way connector; 8) rotatory spanner; 9) nut of three-way connector; 10) locking bracket [ $\phi$ —diameter, the dimensions are given in millimetres (Ed. of Translation)].

The tube was placed in a thermostatted reactor of the high-pressure apparatus and in the course of 7 min the pressure was raised to 2400 kgf cm<sup>-2</sup>. After the experiment the pressure was released, the tube was removed from the reactor, cooled, and washed. The space between the cone of the needle valve and the head was washed through slits cut in the needle. The agreement between the weights of the tube before and after the experiments indicated the absence of leakage of the reaction mixture.